

Single Field Analysis

Name: ani mihailova	ID:	Eye: Left
		DOB: 18-12-2007

Central 30-2 Threshold Test



Fixation Monitor: OFF
 Fixation Target: Central
 Fixation Losses: 0/0
 False POS Errors: 20 %
 False NEG Errors: 17 %
 Test Duration: 12:00

Stimulus: III, White
 Background: 31.5 ASB
 Strategy: SITA-Standard

Pupil Diameter:
 Visual Acuity:
 RX: DS DC X

Date: 30-05-2014
 Time: 16:03
 Age: 6

Fovea: OFF

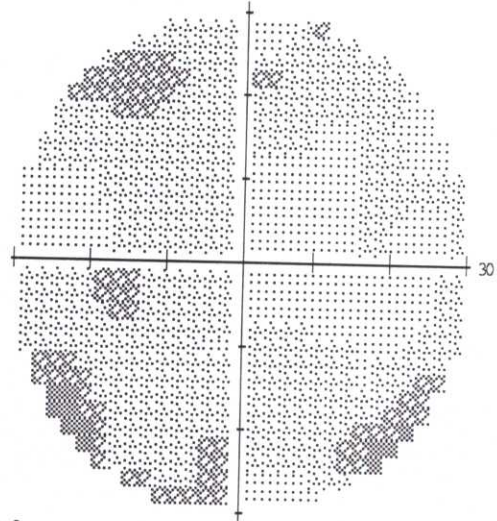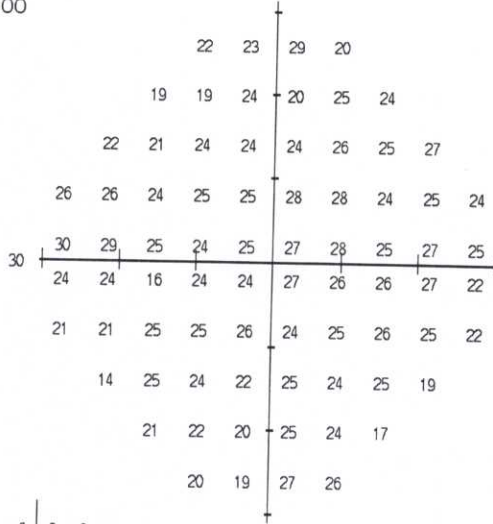


-7	-6	0	-9						
-12	-11	-6	-10	-6	-7				
-10	-10	-8	-8	-9	-6	-7	-5		
-6	-7	-8	-9	-9	-7	-6	-9	-7	-6
-3	-4	-10	-11	-8	-7	-9	-5	-6	
-8	-9	-10	-11	-9	-9	-8	-6	-9	
-11	-11	-9	-9	-9	-11	-9	-7	-7	-9
-19	-8	-9	-11	-9	-9	-7	-12		
-11	-10	-11	-7	-7	-14				
-12	-11	-3	-4						

0	1	7	-3						
-5	-5	0	-4	1	-1				
-4	-4	-2	-2	-3	0	-1	2		
0	0	-2	-2	-3	-1	0	-3	0	0
4	3	-4	-4	-2	0	-2	1	1	
-2	-2	-4	-5	-2	-2	-1	1	-3	
-5	-5	-2	-3	-2	-5	-3	-1	0	-2
-13	-2	-3	-5	-2	-3	-1	-6		
-5	-4	-5	-1	-1	-7				
-5	-5	3	2						


GHT
 General Reduction of Sensitivity

MD -8.57 dB P < 0.5%
 PSD 2.83 dB P < 5%

Total Deviation

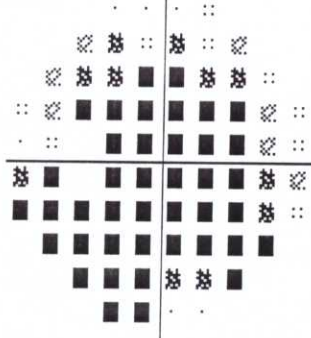

Pattern Deviation

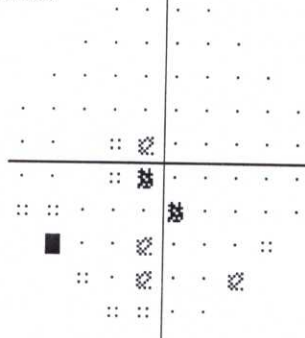

:: < 5%
 ☒ < 2%
 ☒ < 1%
 ■ < 0.5%

SOBAL BURGAS
 Burgas, ul.Alexandrovska 78
 tel (056)-80 11 38 / GSM 0888 212 623
 OLENA Ltd, CARL ZEISS Authorized dealer
 tel.(02)920 1978, fax(02)920 1045

Single Field Analysis

Name: ani mihailova ID: Eye: Right
 Central 30-2 Threshold Test DOB: 18-12-2007



Fixation Monitor: Blindspot
 Fixation Target: Central
 Fixation Losses: 20/21 xx
 False POS Errors: 19 %
 False NEG Errors: 15 %
 Test Duration: 11:41

Stimulus: III, White
 Background: 31.5 ASB
 Strategy: SITA-Standard

Pupil Diameter:
 Visual Acuity:
 RX: DS DC X

Date: 30-05-2014
 Time: 15:43
 Age: 6

Fovea: OFF

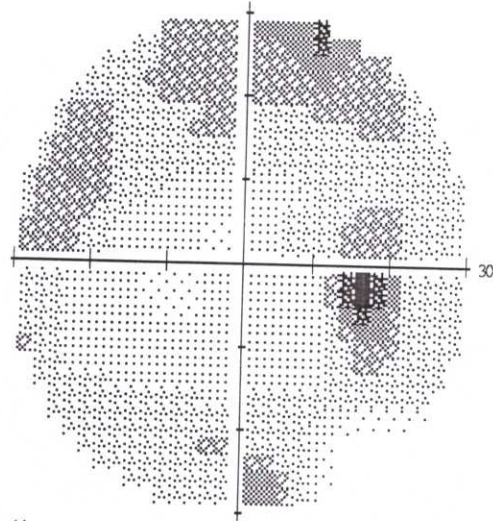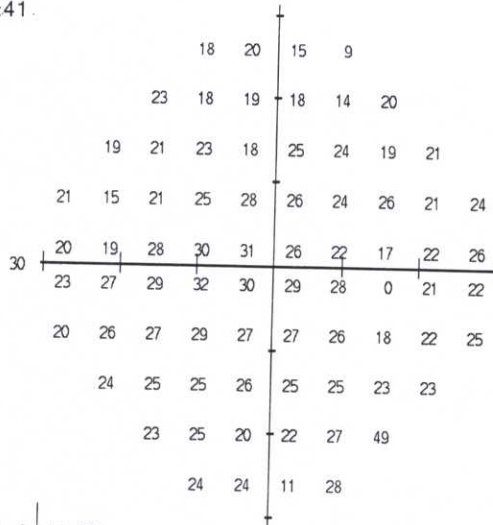


-11	-9	-14	-20						
-8	-13	-12	-13	-17	-10				
-13	-11	-10	-15	-7	-9	-13	-10		
-9	-17	-12	-9	-6	-9	-10	-7	-12	-9
-10	-13	-6	-5	-5	-9	-13	-11	-6	
-8	-6	-5	-3	-6	-6	-7	-12	-10	
-10	-6	-7	-6	-8	-8	-8	-16	-11	-7
-7	-8	-8	-7	-9	-8	-10	-10		
-7	-6	-12	-10	-5	17				
-6	-6	-20	-4						

-5	-3	-8	-14						
-2	-7	-6	-7	-11	-4				
-7	-5	-4	-9	-1	-3	-7	-5		
-4	-11	-7	-3	0	-3	-4	-1	-6	-3
-4	-8	0	1	1	-3	-7	-5	0	
-2	0	1	2	0	-1	-1	-6	-4	
-5	-1	-1	0	-2	-2	-2	-10	-5	-2
-1	-2	-2	-2	-3	-2	-4	-4		
-2	-1	-6	-4	1	23				
0	0	-14	2						


Low Patient Reliability
 GHT
 Outside normal limits

MD -8.23 dB P < 0.5%
 PSD 4.98 dB P < 0.5%

Total Deviation

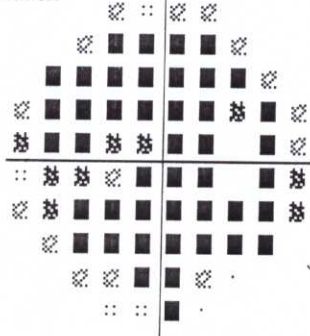

Pattern Deviation

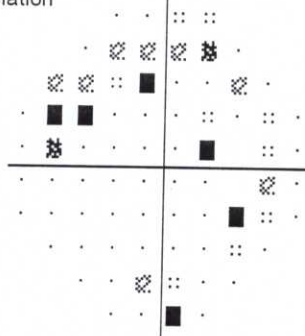

○ < 5%
 ⊙ < 2%
 ⊗ < 1%
 ■ < 0.5%

SOBAL BURGAS

Burgas, ul.Alexandrovska 78
 tel (056)-80 11 38 / GSM 0888 212 623
 OLENA Ltd, CARL ZEISS Authorized dealer
 tel.(02)920 1978, fax(02)920 1045